

V600

Adapt[®] V-Trak

AdaptLift[®] easiSpec

Seating Assessment Specification Form

better comfort all round

incorporating the V-Trak[®] back system

User Weight




User Height

Min: 1560mm
Max: 2100mm



Chair Action

Max height 900mm and tilt (-4° to +20°) all at the touch of a button

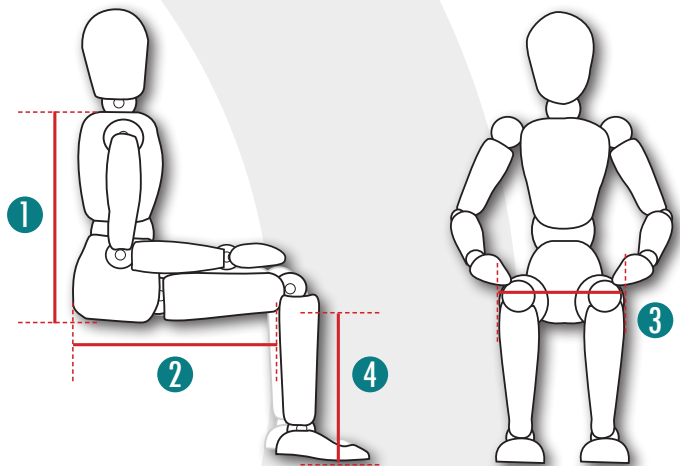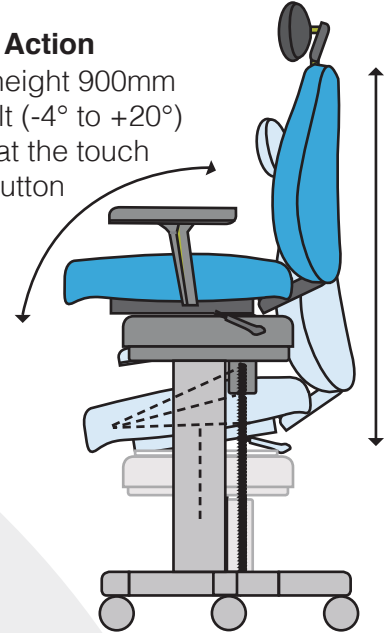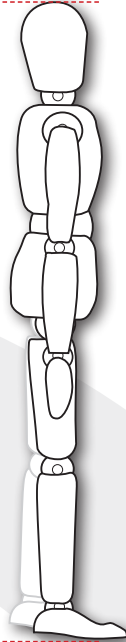

Built-in MLOCK™

AdaptLift also includes a built-in MLOCK™ braking system as standard

- ① Seat to Shoulder (Back Height)
- ② Back of Buttock to Back of Knee (Seat Depth)
- ③ Hip Width at widest point (Seat Width)
- ④ Floor to Underside of Knee (Seat Height - adjustable)

	Min	Max
①	350mm	670mm
②	410mm	610mm
③	410mm	610mm
④	510mm	900mm

Client

Company

Assessor

Date

Seating Assessment / Specification Form


Using the V600 measuring guide, select which of the height scales best matches the back height and axilla height (bearing in mind the lumbar preference) and then select H1, H2, H3 or H4

Then on the reverse side of the measuring guide, select the width option that offers the best wrap support from W1, W2 or W3 and tick the corresponding boxes below

BACK REST



Please tick box option and state the required dimensions if different from those shown

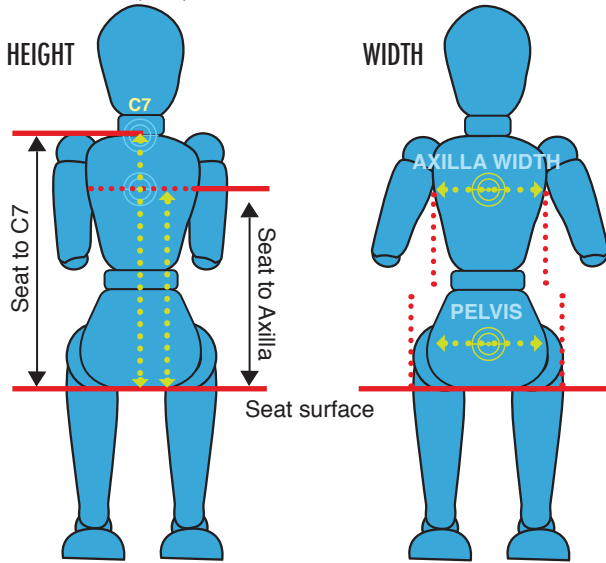

Height from seat to C7
Height from seat to Axilla


Width at Pelvis (inc required wrap for support)
Width at Axilla (inc required wrap for support)

HEIGHT	WIDTH		
	W1	W2	W3
H1	<input type="checkbox"/> 1/1	<input type="checkbox"/> 1/2	<input type="checkbox"/> 1/3
H2	<input type="checkbox"/> 2/1	<input type="checkbox"/> 2/2	<input type="checkbox"/> 2/3
H3	<input type="checkbox"/> 3/1	<input type="checkbox"/> 3/2	<input checked="" type="checkbox"/> N/A
H4	<input checked="" type="checkbox"/> N/A	<input checked="" type="checkbox"/> N/A	<input type="checkbox"/> 4/3

SEAT



Please tick box option and state the required dimensions if different from those shown

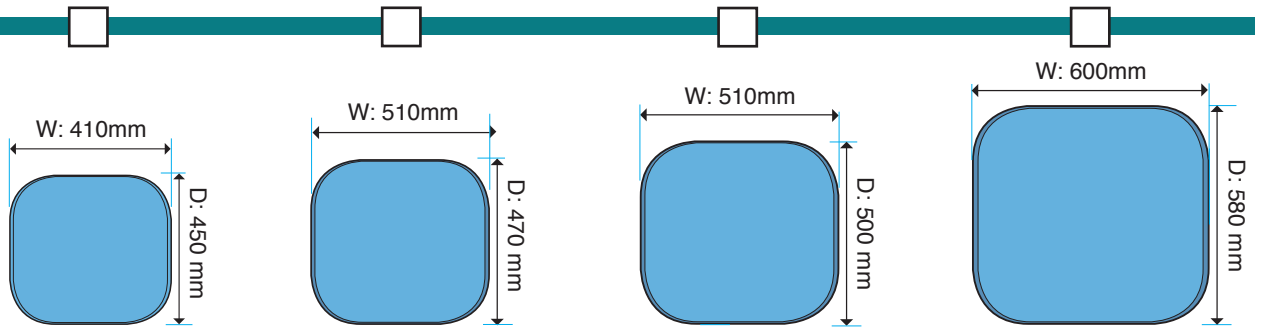

CHAIR CODE

Width Reduction
Depth Reduction


	ALSS	ALSM	ALSL	ALSXL
Width Reduction	Minimum Sizes	REDW: to.....mm	REDW: to.....mm	REDW: to mm
Depth Reduction		REDD: to.....mm	REDD: to.....mm	REDD: to mm

- Use Back of Buttock to Back of Knee measurement and SUBTRACT 30mm to calculate optimum seat depth
- Use Hip to Hip measurement and ADD 50mm to calculate the optimum seat width
- **MINIMUM SEAT WIDTH IS 410mm AND MINIMUM SEAT DEPTH IS 450mm**



Built-in MLOCK™


AdaptLift also includes a built-in MLOCK™ braking system as standard, to hold your chair still when you transfer in and out

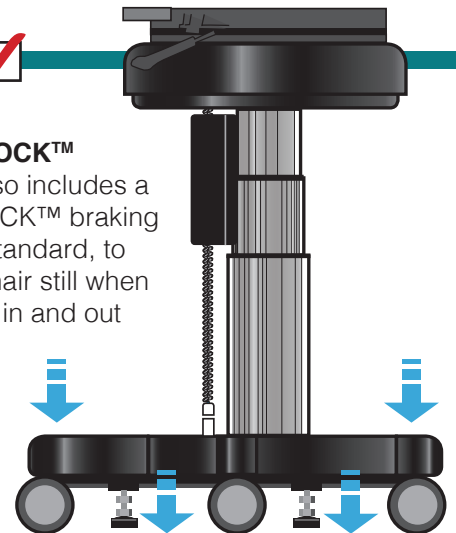

ARM OPTIONS


Level One Adaptations

Please tick required option

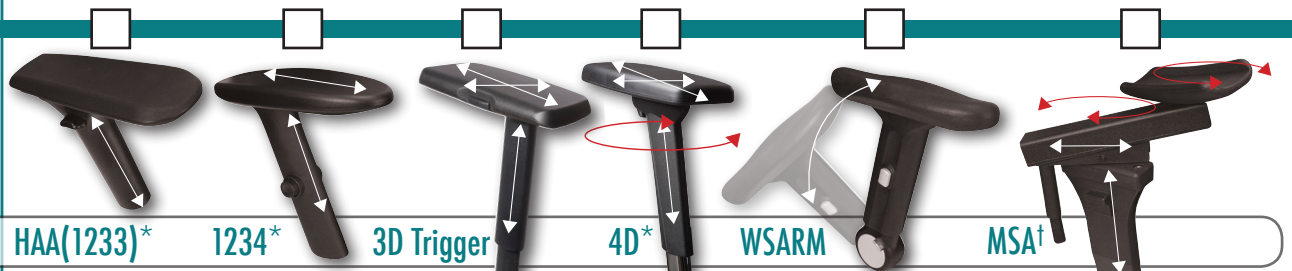

ARM PAD ENHANCEMENTS

Please tick required option

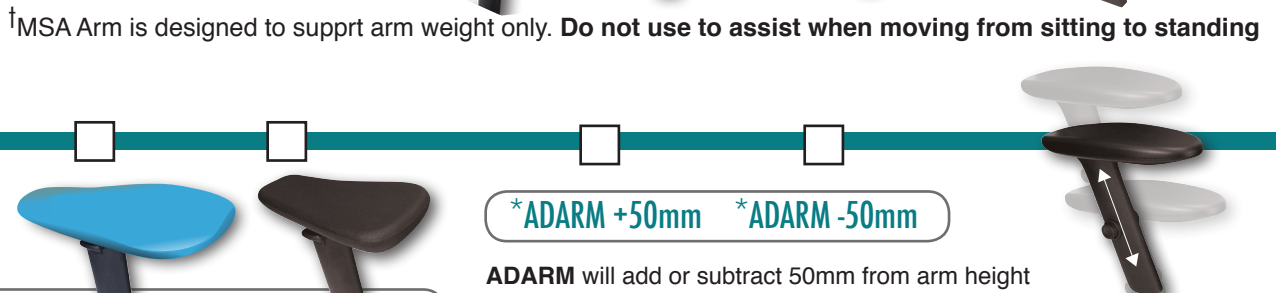


PAD CODE

UPARM GEL PADS

ADARM will add or subtract 50mm from arm height (measured from seat surface to top of arm pad). Applies only to arm options marked with asterisk.

HEAD SUPPORT

Please tick required option

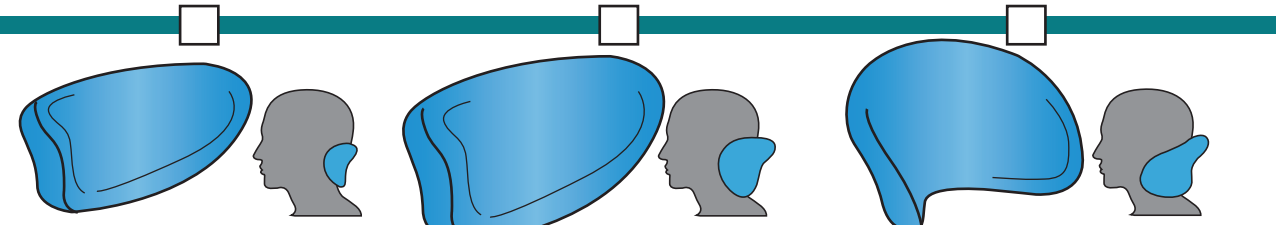


NECK CODE

VTHM VTHL VTHC

SEAT ENHANCEMENT

Level Two Adaptations


Please tick required option

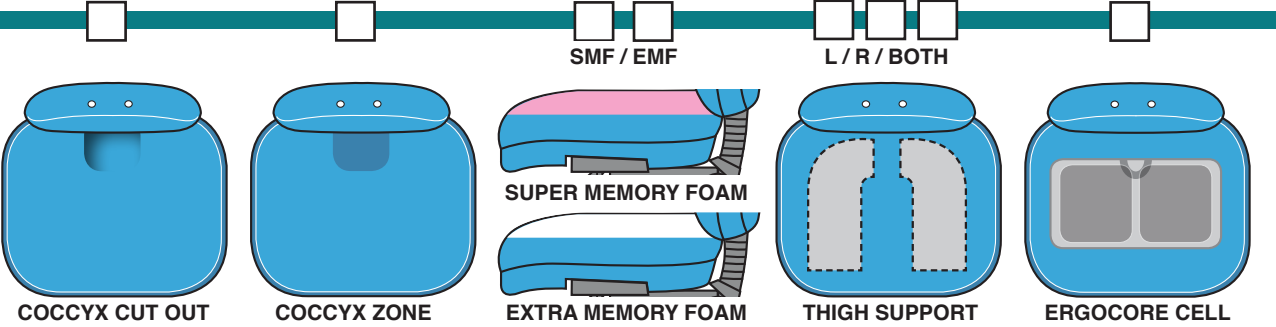

ENHANCE CODE

/CC /CZ SMFS or /MFS /TS /ECORE

Please tick required option

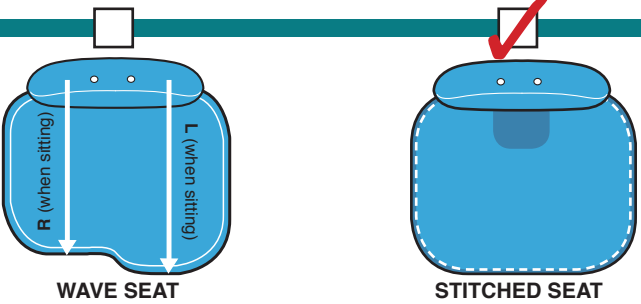

ENHANCE CODE

WAVE SEWN SEAT STANDARD

A sewn seat features as standard and will provide an even thickness of foam and a uniform tension of fabric across the surface of the seat resulting in a superior sit. This is particularly beneficial when specifying extra layers of memory foam in order to achieve a softer sit.


Please specify required WAVE SEAT DEPTH ie. Back Buttock to Back of Knee L&R -30mm
 R (when sitting)mm L (when sitting)mm

**(OPTIONAL)
BACK
ENHANCEMENTS**

Level two Adaptations (continued)

Unless stated otherwise, lumbar cell position will be centered at approx 180mm above seat surface as standard

Please tick box option and state the required dimensions if different from those shown

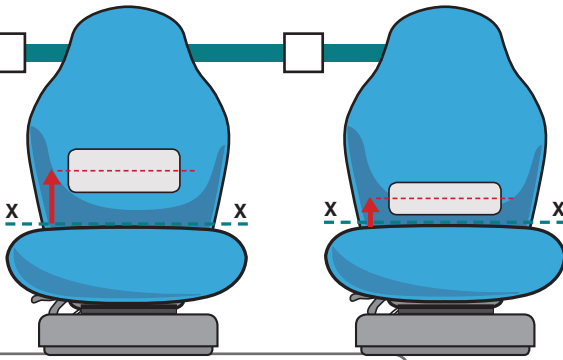

CODE **LUMBAR CELL** **SACRAL CELL**

Measure distance from seat surface to centre of Air Cell and enter as X+



LUMBAR CELL


LOCATE CENTRE OF AIR CELL AT
X+mm

Measure distance from seat surface to centre of Air Cell and enter as X+




SACRAL CELL

LOCATE CENTRE OF AIR CELL AT
X+mm

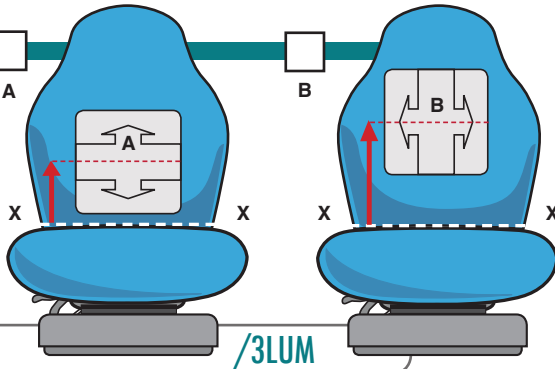


CODE **/3LUM**

Measure distance from seat surface to centre of Air Cell and enter as X+

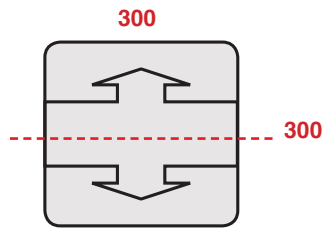

/3LUM REACTIVE LUMBAR CELL


LOCATE CENTRE OF AIR CELL AT
X+mm

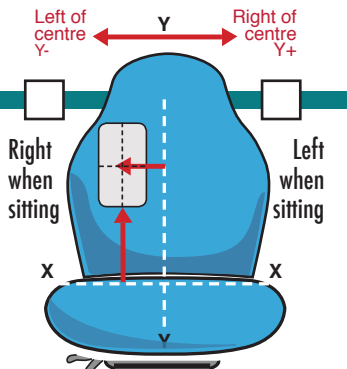

CODE **/VSR** **/VSL**


Measure distance from seat surface to centre of Air Cell and enter as X+

Measure distance from centre of back rest to centre of Air Cell and enter as Y+/-



/VSL /VSR VERTICAL CELL


LOCATE CENTRE OF AIR CELL AT
X+mm
Y+mm
Y-mm

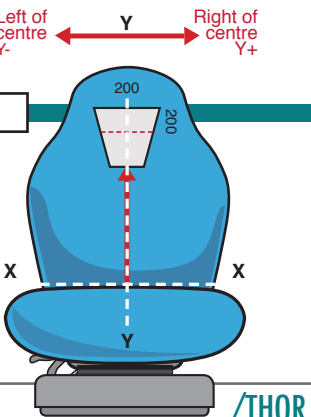

CODE **/THOR**

Measure distance from seat surface to centre of Air Cell and enter as X+

If not using centrally, measure distance from centre of back rest to centre of Air Cell and enter as Y+/-



THORACIC CELL

LOCATE CENTRE OF AIR CELL AT
X+mm
And (if not central)
Y+mm
Y-mm